

CALIBRATION CERTIFICATE

Number **VG250432**

Page 1 of 2

Mettler-Toledo S.A.E.
Laboratorio de Calibración

Carrer Segrià 7 - 9
08940 Cornellà de Llobregat (Barcelona)
Tel. 93 223 76 00
Laboratorio.Calibracion@mt.com

METTLER TOLEDO



ITEM **Piston operated burette**

MANUFACTURER **Mettler Toledo**

MODEL **DV 1005**

NOMINAL VOLUME **5 ml**

IDENTIFICATION **B231174780**

ITEM NUMBER **-**

APPLICANT **Tec Instrumental SA**
Blas Parera 1007
(B1602CTS) Florida-Vte Lopez

Calibration date **01 July 2025**

Authorized Signatory

*This certificate in digital format is the original one.
Any printing will be considered as a copy.*



Este certificado se expide de acuerdo con las condiciones de la acreditación concedida por ENAC, que ha comprobado las capacidades de medida del laboratorio y su trazabilidad a patrones nacionales o internacionales.
ENAC es firmante del Acuerdo de Reconocimiento Mutuo (MLA) de calibración de European Cooperation for Accreditation (EA) y de International Laboratory Accreditation Cooperation (ILAC).
This certificate is issued in accordance with the conditions of accreditation granted by ENAC which has assessed the measurement capability of the laboratory and its traceability to national or international standards.
ENAC is one of the signatories of the Multilateral Agreement of the European Cooperation for Accreditation (EA) and the International Laboratories Accreditation Cooperation (ILAC).

Instrument information

Burette	Mettler Toledo
Serial number	0432
Nominal volume	0,5 ml

Calibration procedure

Procedure PEC/MTE/22 based to the ISO 8655 norm and the METTLER TOLEDO manuals.
The measured volume corresponds with delivered volume (Ex) at the reference temperature of 20 °C.

Calibration conditions

Ambient temperature	Min. 0 °C	Max. 0 °C
Relative humidity	% Hr % Hr	
Pressure	Presión atm. mbar	

Maintenance: Before calibration, seals (references 101003 and 25737) and piston have been replaced, and burette glass has been cleaned.

Traceability

Standard equipment used		
Balance	BAL01	AT201 - 5 decimal places balance
Burette drive	VAL-T50	T50
Water temperature	TER 144	0,1 °C resolution
Ambient conditions	REG05	(air Temp, rH)
Class III water	2419109811	


The measured volume has been calculated conform to ISO/TR 20461:2023.
The traceability of measurements are referred to laboratories accredited by ILAC signatories accreditation bodies or national laboratories EURAMET signatories.

Uncertainty

The reported expanded measurement uncertainty is stated as the standard measurement uncertainty multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 %.

Calibration results (after maintenance)

Burette stroke	10%	30%	50%	100%	
Selected volume	0,5	1,5	2,5	5	ml
Water temperature	19,8	19,8	19,8	19,8	°C
Measured volume	499,7	1499,8	2500,5	5000,1	µl
Systematic error	-0,3	-0,2	0,5	0,1	µl
Measurement uncertainty	2,5	2,5	2,5	2,5	µl
Random error	0,22	0,11	0,27	0,23	µl
Max. Permissible Sys. Error	15	15	15	15	µl
Max. Permissible Random Error	5	5	5	5	µl
Evaluation*	Pass	Pass	Pass	Pass	

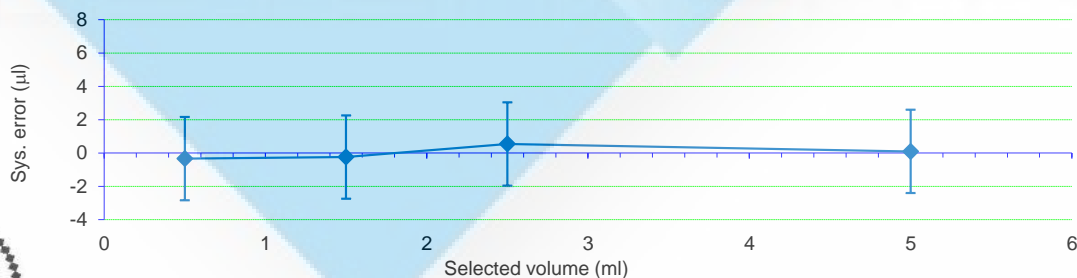

* Evaluation and permissible errors from ISO 8655-3:2022. According with this norm, uncertainty is not taken into account.

Mettler- Toledo S.A.E.

Carrer Segrià, 7-9
08940 Cornellà de Llobregat (Barcelona)

Technician: P.Cuenca
Remarks: ---